LFPSE Event flow

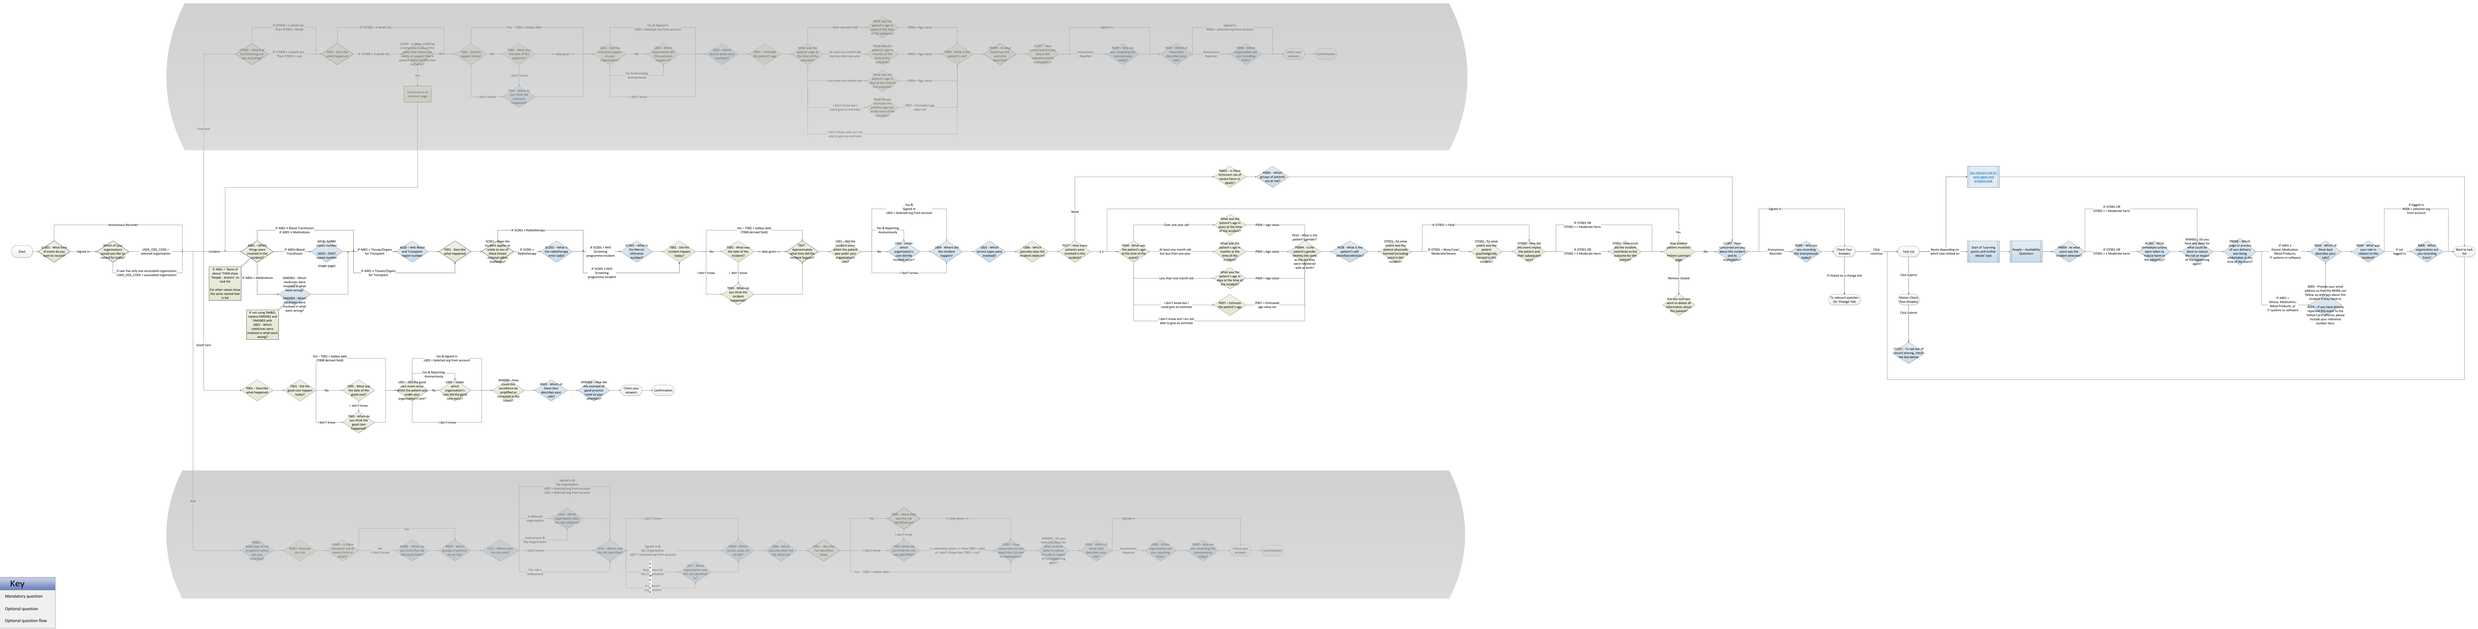

People - Availability

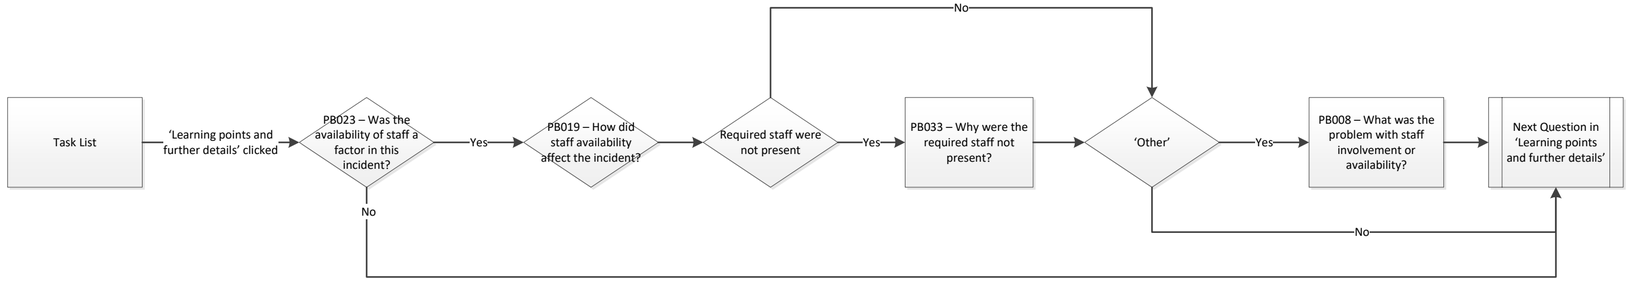

People - Activites

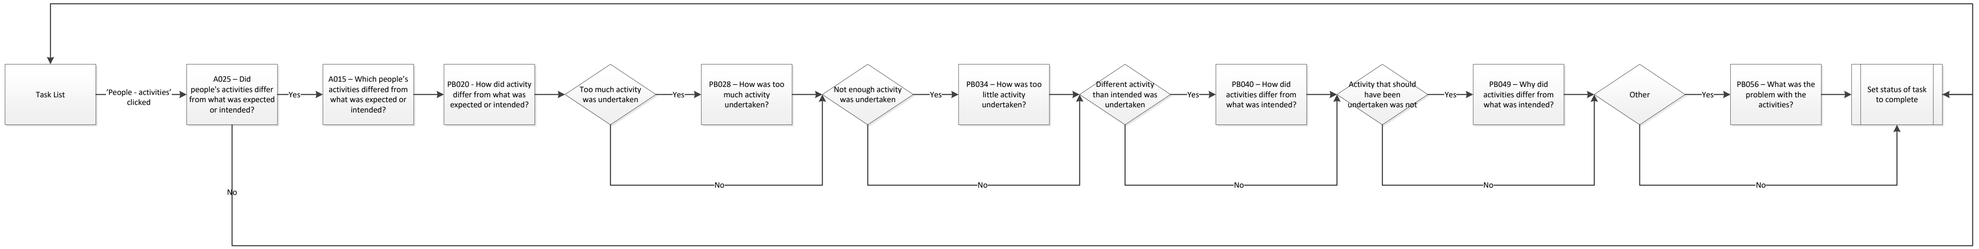

Devices

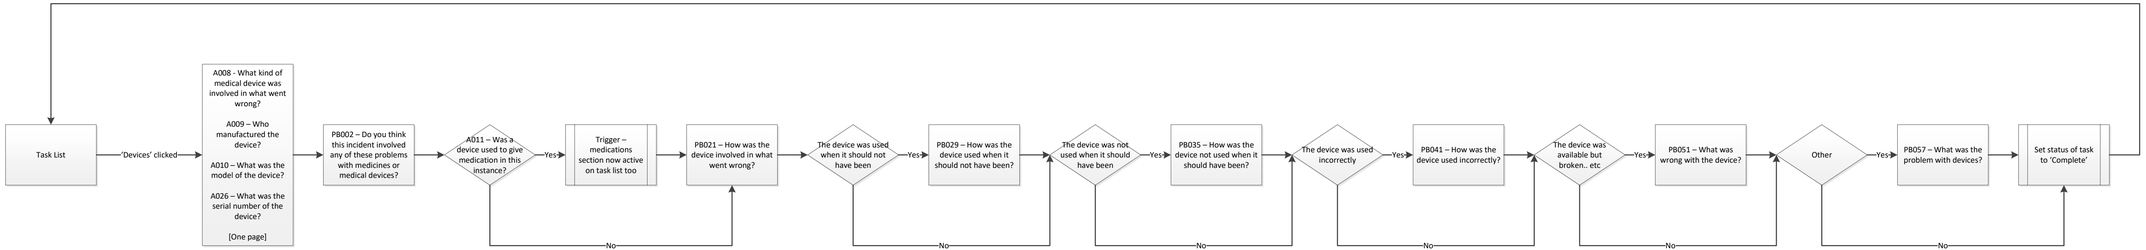
Task List
'Devices' clicked
A008 - What kind of medical device was involved in what went wrong?
A009 – Who manufactured the device?
A010 – What was the model of the device?
A026 – What was the serial number of the device?
[One page]
PB002 – Do you think this incident involved any of these problems with medicines or medical devices?
A011 – Was a device used to give medication in this instance?
Yes
Trigger – medications section now active on task list too
No
PB021 – How was the device involved in what went wrong?
The device was used when it should not have been
Yes
PB029 – How was the device used when it should not have been?
No
The device was not used when it should have been
Yes
PB035 – How was the device not used when it should have been?
No
The device was used incorrectly
Yes
PB041 – How was the device used incorrectly?
No
The device was available but broken.. etc
Yes
PB051 – What was wrong with the device?
No
Other
Yes
PB057 – What was the problem with devices?
No
Set status of task to 'Complete'

Medications

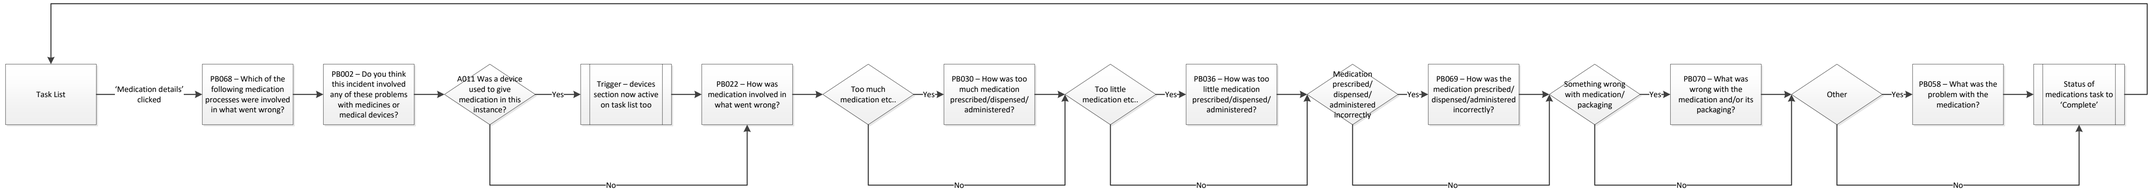

IT Systems

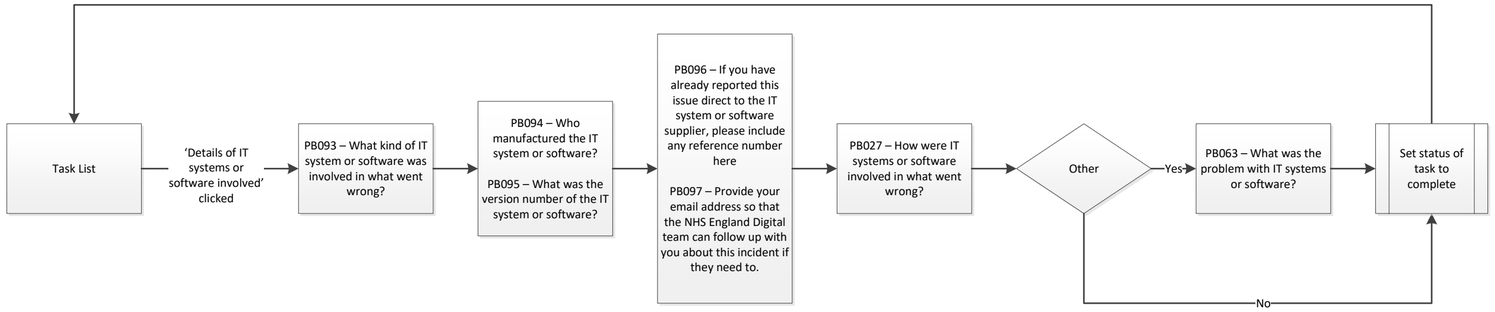
Task List
'Details of IT systems or software involved' clicked
PB093 – What kind of IT system or software was involved in what went wrong?
PB094 – Who manufactured the IT system or software?
PB095 – What was the version number of the IT system or software?
PB096 – If you have already reported this issue direct to the IT system or software supplier, please include any reference number here
PB097 – Provide your email address so that the NHS England Digital team can follow up with you about this incident if they need to.
PB027 – How were IT systems or software involved in what went wrong?
Other
Yes
PB063 – What was the problem with IT systems or software?
Set status of task to complete
No

Buildings or Infrastructure

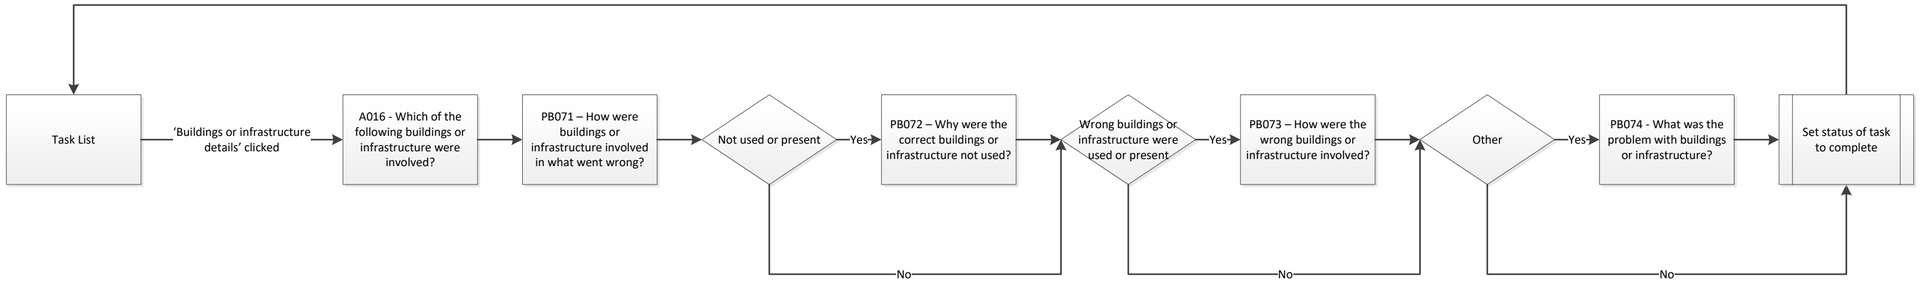

Estates Services

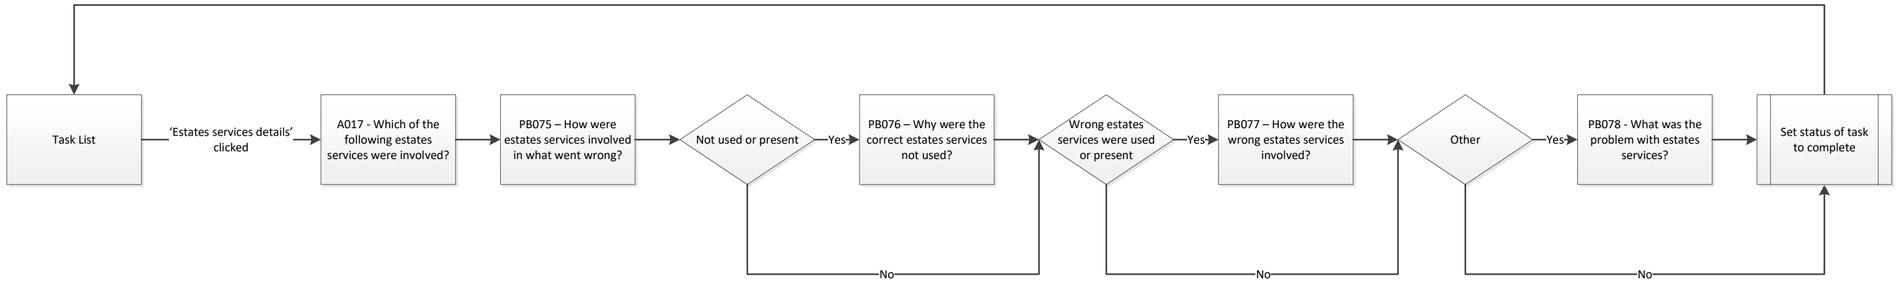

Blood transfusion

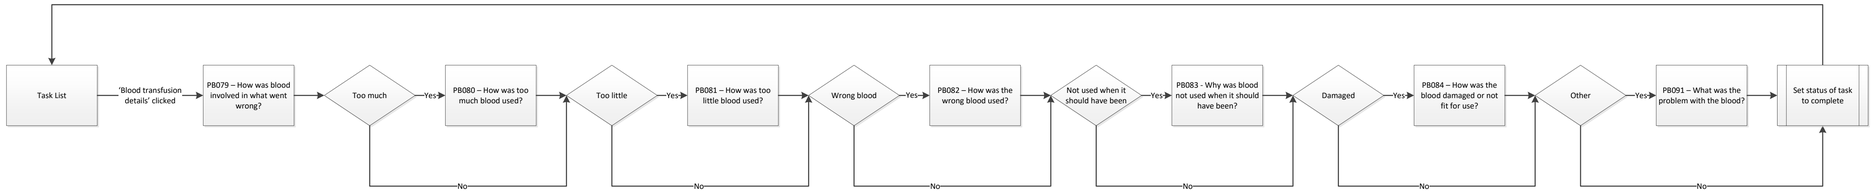

Blood Products

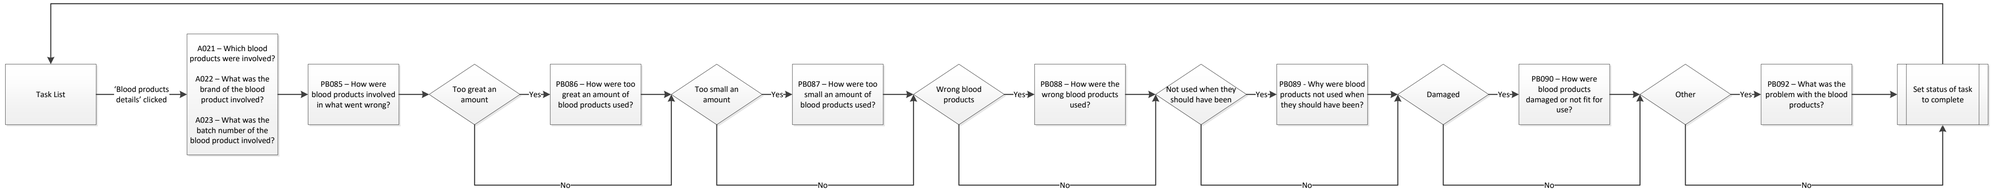

Tissues or Organs for Transplant

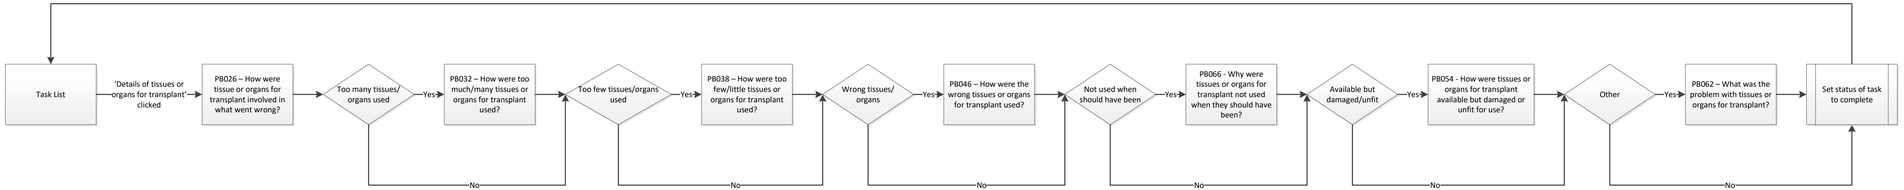
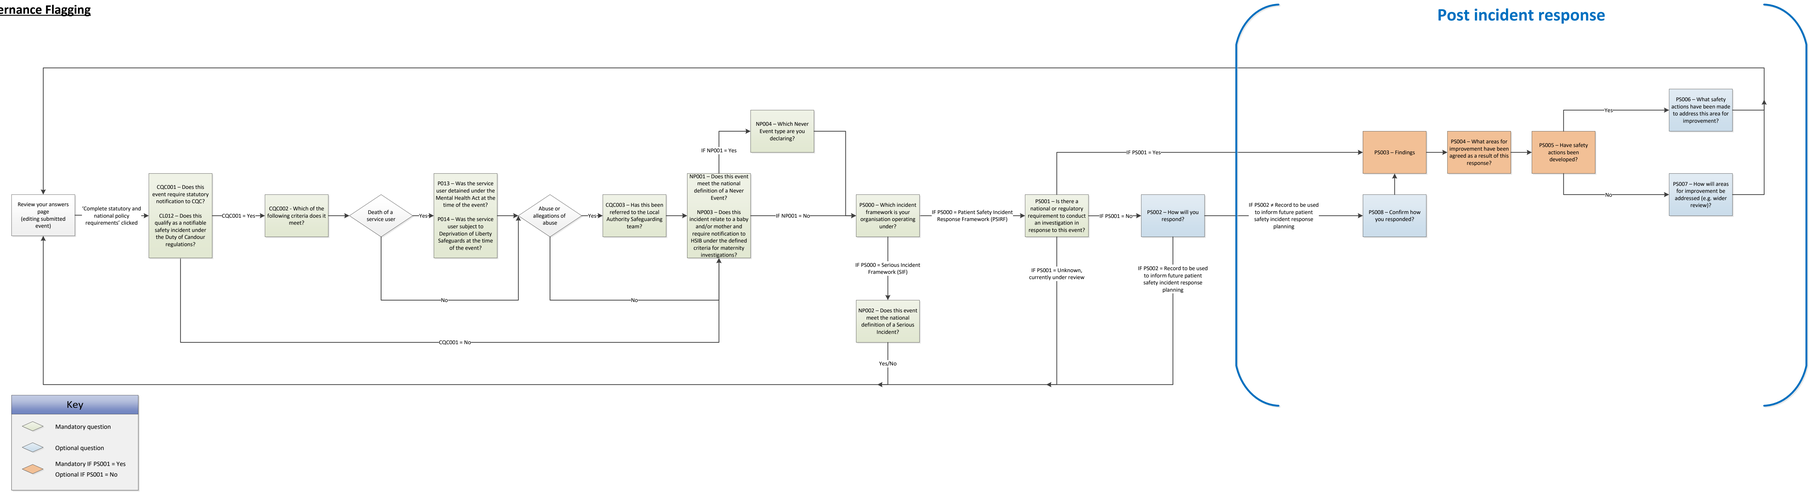
Governance Flagging